



All Faculty Publications

2005-12-30

Analysis of Grain Screenings by X-ray Photoelectron Spectroscopy

Guilin Jiang

Brigham Young University - Provo

Ghaleb A. Hussein

Brigham Young University - Provo

See next page for additional authors

Follow this and additional works at: <https://scholarsarchive.byu.edu/facpub>

 Part of the [Chemical Engineering Commons](#)

Original Publication Citation

Jiang, G., Hussein, G. A., Baxter, L. L., & Linford, M. R. (2005). Analysis of grain screenings by x-ray photoelectron spectroscopy. *Surface Science Spectra*, 11(1): 97-104.

BYU ScholarsArchive Citation

Jiang, Guilin; Hussein, Ghaleb A.; Baxter, Larry Lin; and Linford, Matthew R., "Analysis of Grain Screenings by X-ray Photoelectron Spectroscopy" (2005). *All Faculty Publications*. 1734.
<https://scholarsarchive.byu.edu/facpub/1734>

This Peer-Reviewed Article is brought to you for free and open access by BYU ScholarsArchive. It has been accepted for inclusion in All Faculty Publications by an authorized administrator of BYU ScholarsArchive. For more information, please contact scholarsarchive@byu.edu, ellen_amatangelo@byu.edu.

Authors

Guilin Jiang, Ghaleb A. Hussein, Larry Lin Baxter, and Matthew R. Linford

Analysis of Grain Screenings by X-ray Photoelectron Spectroscopy

Guilin Jiang, Ghaleb A. Hussein,^{a)} Larry L. Baxter, and Matthew R. Linford
Brigham Young University, Provo, Utah 84604

(Received 12 August 2004; accepted 16 November 2005; published 30 December 2005)

Determining the chemical structure and composition of biomass fuels using x-ray photoelectron spectroscopy (XPS) can provide fundamental knowledge of their structures that is useful in understanding and predicting their combustion behavior. Grain screenings are an example of an agricultural residue (byproduct of food and feed production) of potential interest for biomass combustion. The XPS spectra of grain screenings provide both its elemental composition and indications of its bonding. Traditional fuel analyses of this fuel are also provided. These include: ultimate analysis — the elemental composition of the overall fuel (C, H, N, S, and O); chlorine analysis — reported here as part of the ultimate analysis but formally a separate procedure; proximate analysis — the proximate composition of the fuel (moisture, fixed carbon, volatiles, and ash); heating value — the specific heat of combustion; ash chemistry analysis — an elemental analysis of the ash content, expressed as oxides (which does not imply that they occur as oxides in the fuel). These data are summarized with the XPS spectra. © 2005 American Vacuum Society. [DOI: 10.1116/11.20040802]

Keywords: biomass; grain screenings; XPS; fuel

PACS: 82.80.Pv, 01.30.Kj, 84.60.Rb, 82.33.Vx, 82.60.Cx

SPECIMEN DESCRIPTION

Host Material: grain screenings

Host Material Characteristics: homogeneous; amorphous; unknown electrical characteristics; biological material; powder

Chemical Name: cellulose

Host Composition: see entry for History & Significance

Form: powder

History & Significance: Grain screenings are an example of an agricultural residue (byproduct of food and feed production) of potential interest for biomass combustion. The XPS spectra of grain screenings provide both its elemental composition and indications of its bonding.

Traditional fuel analyses of this fuel are also provided. These include: ultimate analysis — the elemental composition of the overall fuel (C, H, N, S, and O); chlorine analysis — reported here as part of the ultimate analysis but formally a separate procedure; proximate analysis — the proximate composition of the fuel (moisture, fixed carbon, volatiles, and ash); heating value — the specific heat of combustion; ash chemistry analysis — an elemental analysis of the ash content, expressed as oxides (which does not imply that they occur as oxides in the fuel). These data are summarized with the XPS spectra. The chemical composition of grain screenings is summarized in Tables 1 and 2.

As Received Condition: powder

Analyzed Region: same as host material

Ex Situ Preparation/Mounting: Sawdust powders were used as received. The powders were pressed onto a piece of nonconductive double-sticky tape mounted on a piece of silicon,

^{a)}Author to whom correspondence should be addressed; present address: Chemical Engineering Department, P.O. Box 26666, The American University of Sharjah, Sharjah, United Arab Emirates.

Accession # 00896

Technique: XPS

Host Material: grain screenings

Instrument: Surface Science Instruments SSX-100

Major Elements in Spectrum: C, O

Minor Elements in Spectrum: N, Si

Printed Spectra: 8

Spectra in Electronic Record: 8

Spectral Category: technical

Table 1: Fuel analysis of bio-fuel grain screenings (ash free basis except for ash and LHV, which are on an as-received basis).

	% by weight
Moisture	11.47
C	41.00
H	5.60
O	31.61
N	1.83
S	0.22
Ash	8.27
Sum	100.0
LHV*, MJ/kg	16.397

* Lower heating value

Table 2: Ash composition of grain screenings (percent of ash basis).

	Mass %
SiO ₂	34.4
Al ₂ O ₃	2.2
Fe ₂ O ₃	2.6
CaO	15.8
MgO	3.9
Na ₂ O	1.9
K ₂ O	19.2
SO ₃	5.1
P ₂ O ₅	11.6
Cl	2.8
Other	0.5
Sum	100

which was then mounted on the sample stage with a piece of the same tape.

In Situ Preparation: none

Pre-Analysis Beam Exposure: No damage was observed in the sample even after several hours of exposure to x-ray radiation. After 4 h of exposure to x rays, the intensity of the N 1s scan did not change.

Charge Control: A flood gun was applied. The flood gun voltage was 4 V, and its current was less than 50 mA. A metal screen was used to mask the sample. The charge control was determined by observing zirconia Zr 3p_{3/2} peak positions under different flood gun settings. XPS spectra showed a Zr 3d_{5/2} at 182.3 eV. The metal screen used was nickel, 1 mm distance, 70 lines/in. and 90% transmission.

Temp. During Analysis: 298 K

Pressure During Analysis: $<2.0 \times 10^{-6}$ Pa

INSTRUMENT DESCRIPTION _____

Manufacturer and Model: Surface Science Instruments SSX-100

Analyzer Type: spherical sector

Detector: resistive anode position detector

Number of Detector Elements: 128

INSTRUMENT PARAMETERS COMMON TO ALL SPECTRA

■ **Spectrometer**

Analyzer Mode: constant pass energy

Throughput ($T = E^N$): $N=0$

Excitation Source Window: 12 μ m aluminum foil

Excitation Source: Al K $_{\alpha}$ monochromatic

Source Energy: 1486.6 eV

Source Strength: 200 W

Signal Mode: multichannel direct

■ **Geometry**

Incident Angle: 55°

Source to Analyzer Angle: 70.8°

Emission Angle: 55°

Specimen Azimuthal Angle: 0°

Acceptance Angle from Analyzer Axis: 0°

DATA ANALYSIS METHOD _____

Peak Shape and Background Method: Shirley background function

Quantitation Method: Sensitivity factors were obtained from ESCA 2000 NT software supplied by Service Physics. The peak areas are the areas above a linear background.

ACKNOWLEDGMENTS _____

The authors acknowledge U.S. DOE Biomass Power Program for financial support, and Elsam engineering and Eltra, both Danish companies, which provided complementary analyses and some financial support for this investigation.

SPECTRAL FEATURES TABLE

Spectrum ID #	Element/ Transition	Peak Energy (eV)	Peak Width FWHM (eV)	Peak Area (counts)	Sensitivity Factor	Concentration (at. %)	Peak Assignment
00896-02	O 1s	528.5	4.0	8400	2.5	14.9	...
00896-03	C 1s	280.9	2.7	92600	1	81.7	...
00896-04	N 1s	396.3	4.5	26300	1.68	1.4	...
00896-05	Si 2p	99.3	4.7	4100	0.9	2	...
00896-06	O 1s	528.6	3.4	22200	2.5
00896-07	C 1s	280.7	1.4	28200	1
00896-08	N 1s	396.2	4.1	21100	1.68


GUIDE TO FIGURES

Spectrum (Accession) #	Spectral Region	Voltage Shift*	Multiplier	Baseline	Comment #
896-1	Survey	0	1	0	1
896-2	O 1s	0	1	0	1
896-3	C 1s	0	1	0	1
896-4	N 1s	0	1	0	1
896-5	Si 2p	0	1	0	1
896-6	O 1s	0	1	0	2
896-7	C 1s	0	1	0	2
896-8	N 1s	0	1	0	2


* Voltage shift of the archived (as-measured) spectrum relative to the printed figure. The figure reflects the recommended energy scale correction due to a calibration correction, sample charging, flood gun, or other phenomenon.

1. 800 μm x-ray beam diameter, 150 eV pass energy

2. 300 μm x-ray beam diameter, 50 eV pass energy

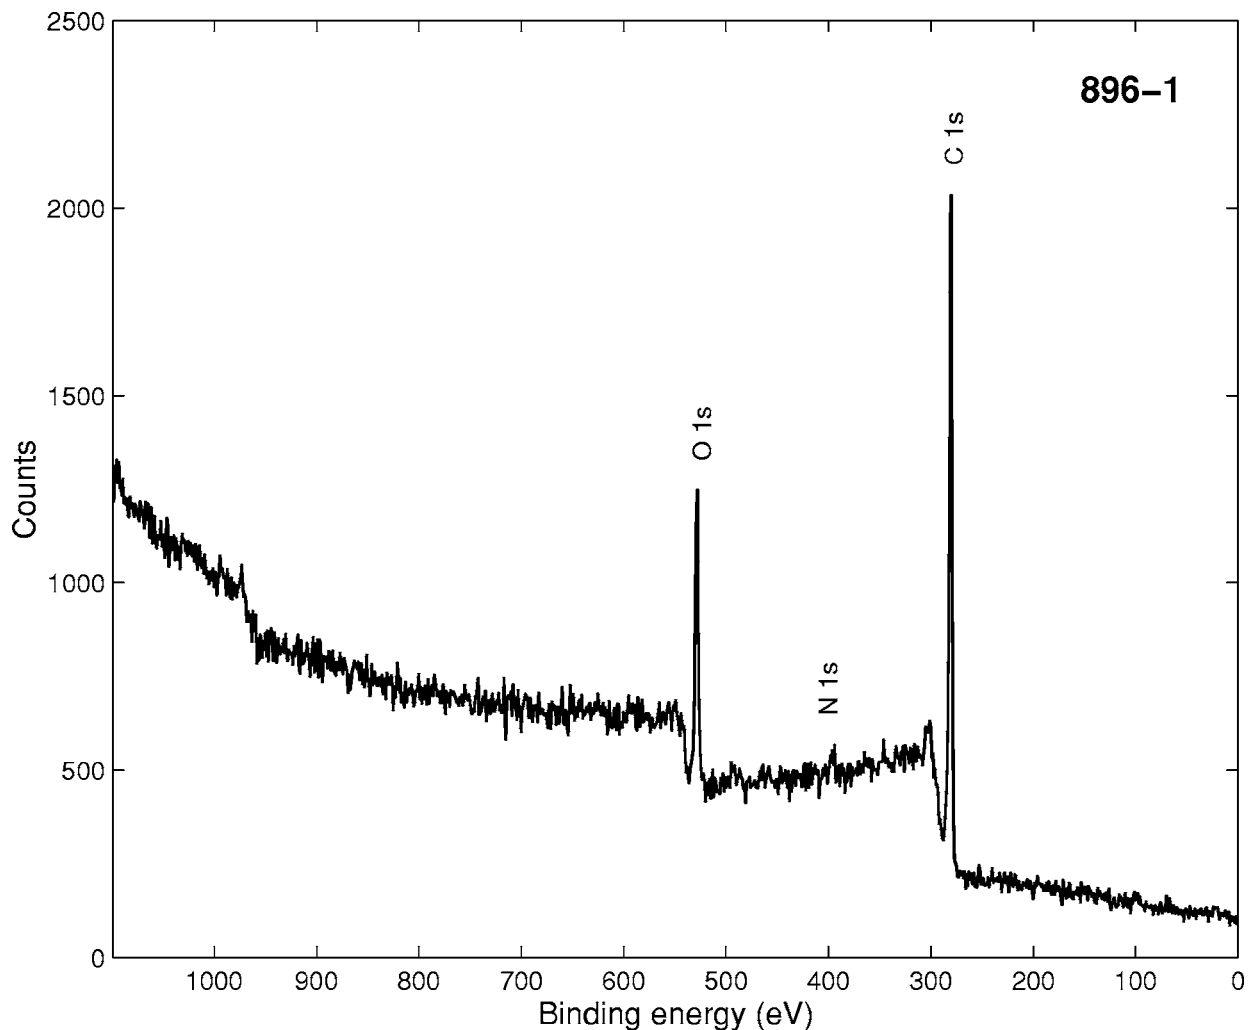


Accession #	00896-01
Host Material	grain screenings
Technique	XPS
Spectral Region	survey
Instrument	Surface Science Instruments SSX-100
Excitation Source	Al K_{α} monochromatic
Source Energy	1486.6 eV
Source Strength	200 W
Source Size	0.8 mm \times 0.8 mm
Analyzer Type	spherical sector
Incident Angle	55°
Emission Angle	55°
Analyzer Pass Energy	150 eV
Analyzer Resolution	1.5 eV
Total Signal Accumulation Time	1100 s
Total Elapsed Time	1300 s
Number of Scans	5
Source Beam Size at Specimen Surface	0.8 mm \times 1.392 mm
Effective Detector Width	19 eV
Analyzer Width	1500 μ m \times 12000 μ m at 84 eV

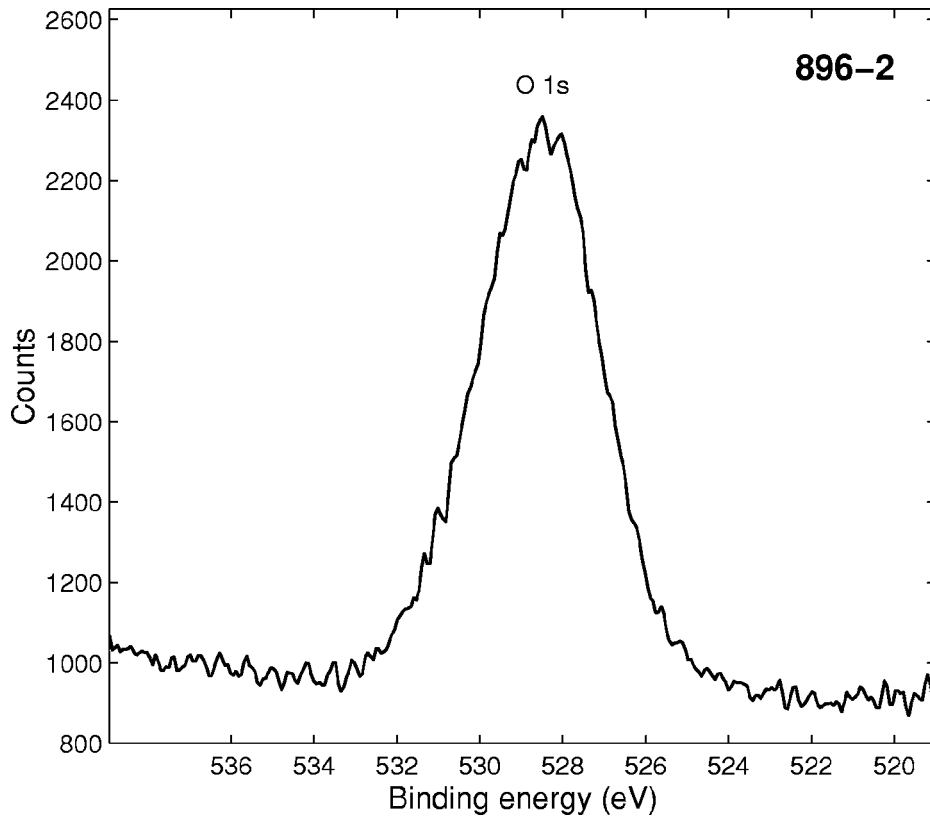


■ **Accession #:** 00896-02
 ■ **Host Material:** grain screenings
 ■ **Technique:** XPS
 ■ **Spectral Region:** O 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 200 W
 Source Size: 0.8 mm \times 0.8 mm
 Incident Angle: 55°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 150 eV
 Analyzer Resolution: 1.5 eV
 Emission Angle: 55°
 Total Signal Accumulation Time: 613 s
 Total Elapsed Time: 472 s
 Number of Scans: 10
 Source Beam Size at Specimen Surface: 0.8 mm \times 1.392 mm
 Effective Detector Width: 19 eV
 Analyzer Width: 1500 μm \times 12000 μm at 84 eV

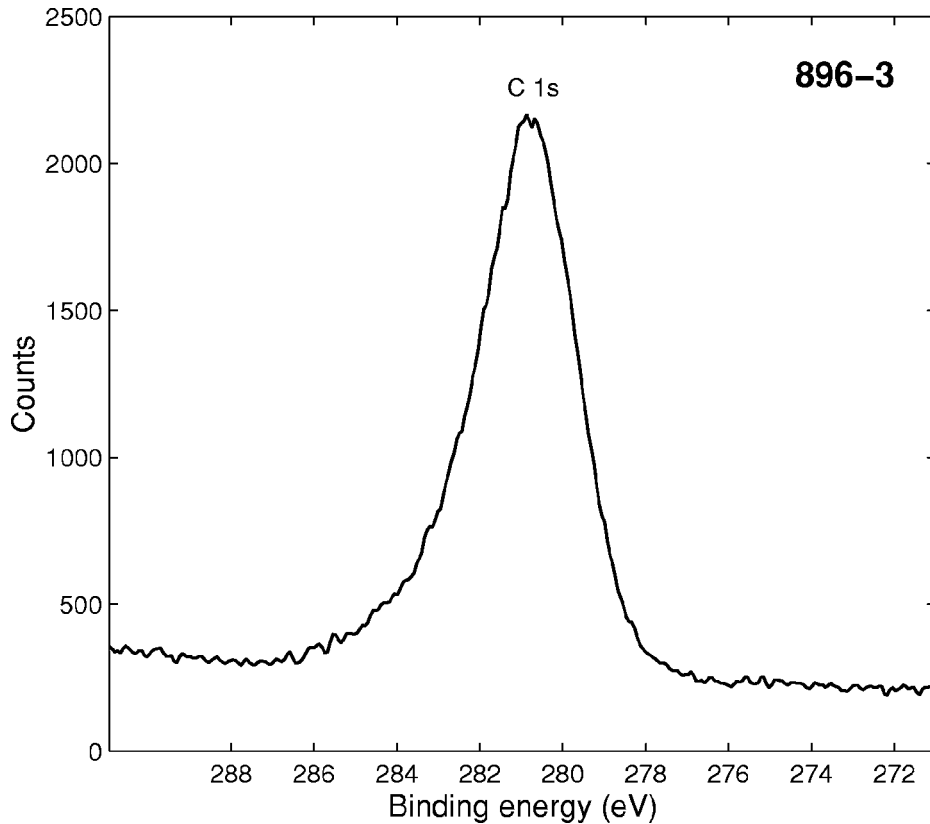


■ **Accession #:** 00896-03
 ■ **Host Material:** grain screenings
 ■ **Technique:** XPS
 ■ **Spectral Region:** C 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 200 W
 Source Size: 0.8 mm \times 0.8 mm
 Incident Angle: 55°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 150 eV
 Analyzer Resolution: 1.5 eV
 Emission Angle: 55°
 Total Signal Accumulation Time: 306.5 s
 Total Elapsed Time: 475.5 s
 Number of Scans: 5
 Source Beam Size at Specimen Surface: 0.8 mm \times 1.392 mm
 Effective Detector Width: 19 eV
 Analyzer Width: 1500 μm \times 12000 μm at 84 eV

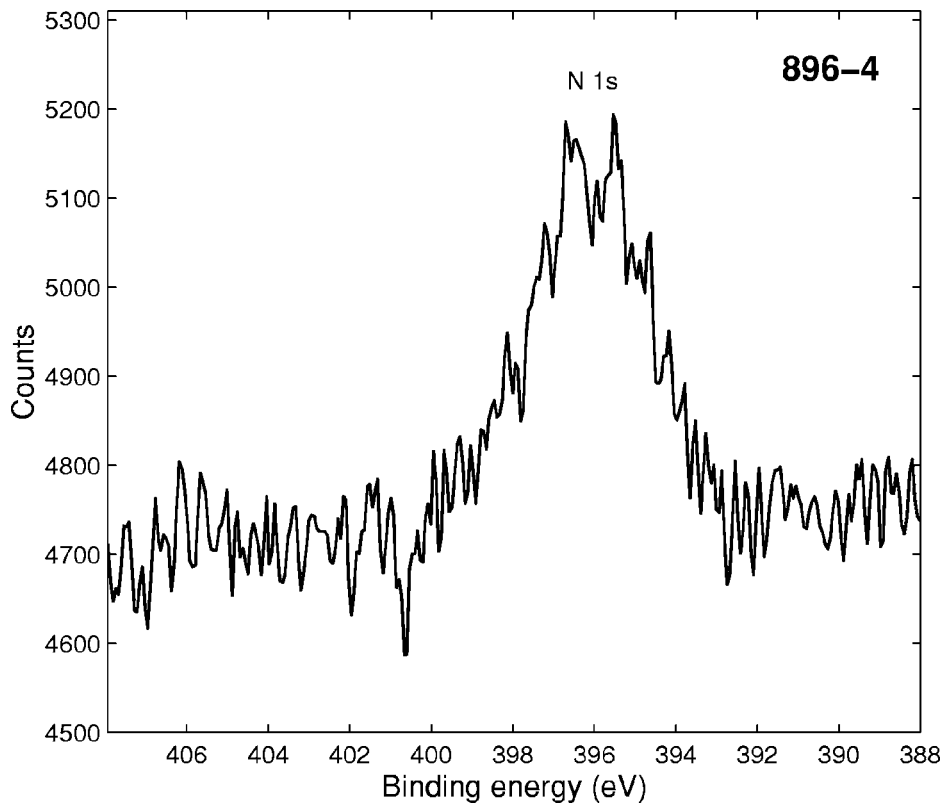


■ **Accession #:** 00896-04
 ■ **Host Material:** grain screenings
 ■ **Technique:** XPS
 ■ **Spectral Region:** N 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 200 W
 Source Size: 0.8 mm \times 0.8 mm
 Incident Angle: 55°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 150 eV
 Analyzer Resolution: 1.5 eV
 Emission Angle: 55°
 Total Signal Accumulation Time: 3065 s
 Total Elapsed Time: 3234 s
 Number of Scans: 50
 Source Beam Size at Specimen Surface: 0.8 mm \times 1.392 mm
 Effective Detector Width: 19 eV
 Analyzer Width: 1500 μm \times 12000 μm at 84 eV

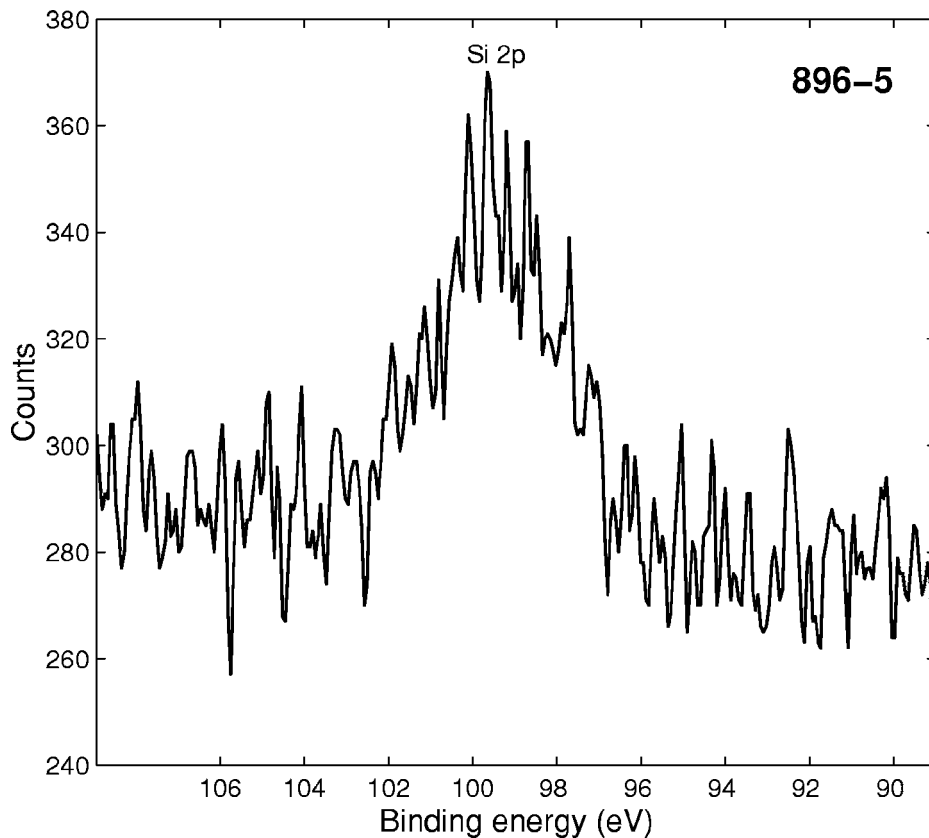


■ **Accession #:** 00896-05
 ■ **Host Material:** grain screenings
 ■ **Technique:** XPS
 ■ **Spectral Region:** Si 2p

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 200 W
 Source Size: 0.8 mm \times 0.8 mm
 Incident Angle: 55°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 150 eV
 Analyzer Resolution: 1.5 eV
 Emission Angle: 55°
 Total Signal Accumulation Time: 613 s
 Total Elapsed Time: 782 s
 Number of Scans: 10
 Source Beam Size at Specimen Surface: 0.8 mm \times 1.392 mm
 Effective Detector Width: 19 eV
 Analyzer Width: 1500 μm \times 12000 μm at 84 eV

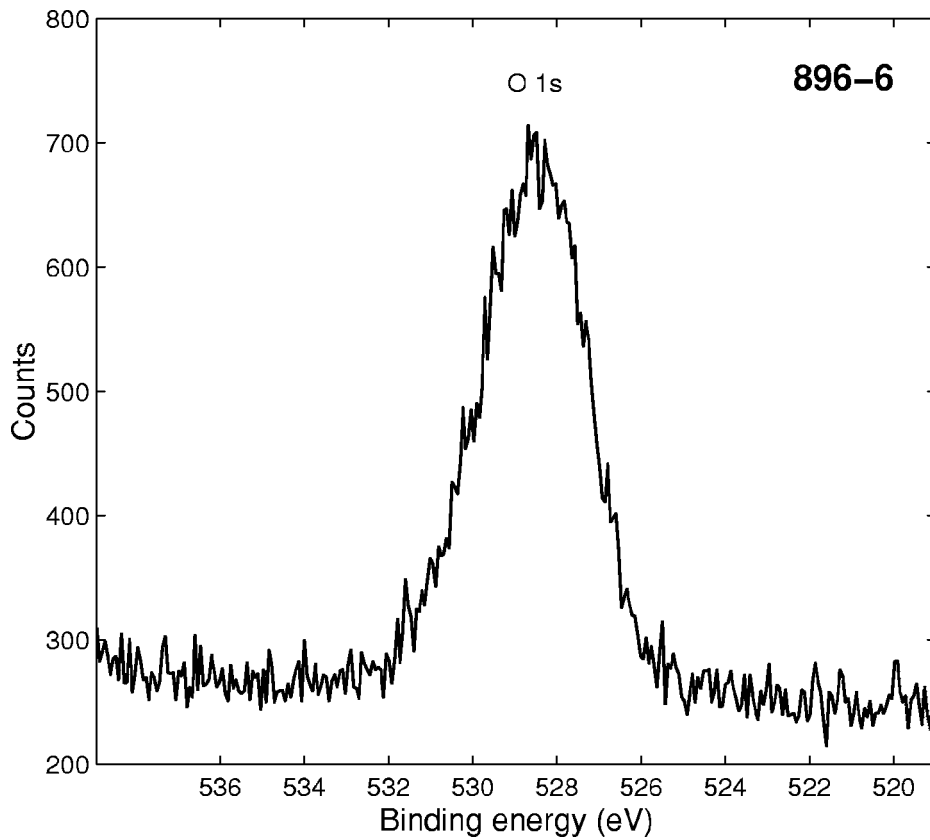


■ **Accession #:** 00896-06
 ■ **Host Material:** grain screenings
 ■ **Technique:** XPS
 ■ **Spectral Region:** O 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 200 W
 Source Size: 0.3 mm \times 0.3 mm
 Incident Angle: 55°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 50 eV
 Analyzer Resolution: 0.5 eV
 Emission Angle: 55°
 Total Signal Accumulation Time: 1226 s
 Total Elapsed Time: 1395 s
 Number of Scans: 20
 Source Beam Size at Specimen Surface: 0.3 mm \times 0.523 mm
 Effective Detector Width: 6.6 eV
 Analyzer Width: 750 μ m \times 6000 μ m

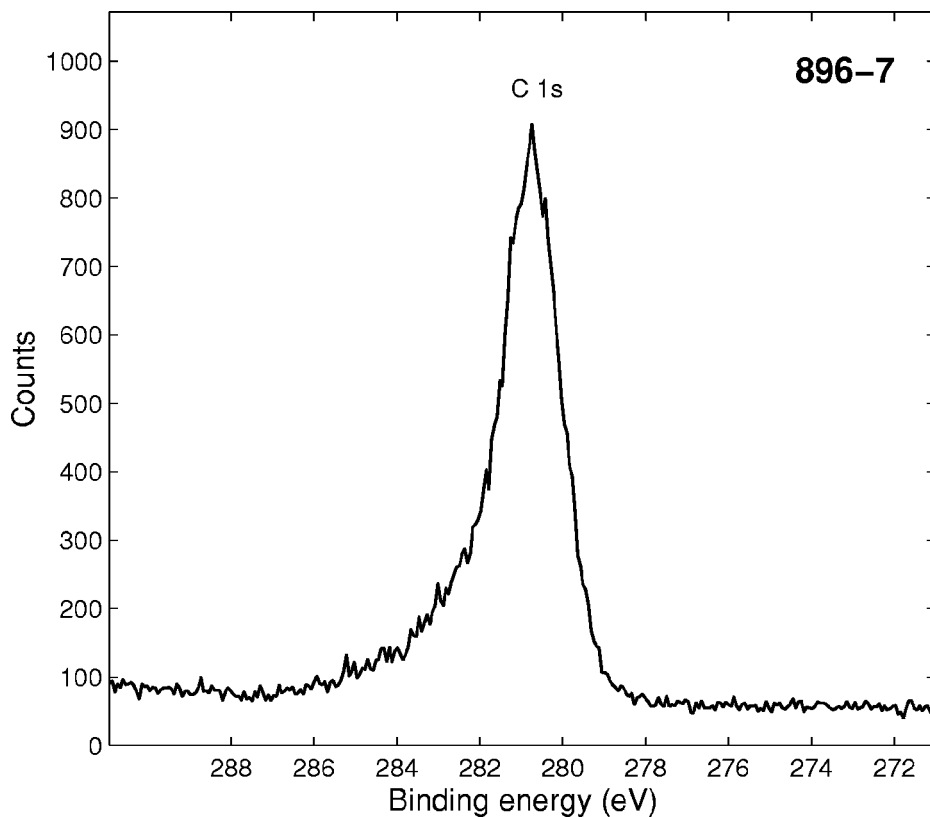

■ **Accession #:** 00896-07
 ■ **Host Material:** grain screenings
 ■ **Technique:** XPS
 ■ **Spectral Region:** C 1s

Instrument: Surface Science Instruments SSX-100
 Excitation Source: Al K_{α} monochromatic
 Source Energy: 1486.6 eV
 Source Strength: 200 W
 Source Size: 0.3 mm \times 0.3 mm
 Incident Angle: 55°
 Analyzer Type: spherical sector
 Analyzer Pass Energy: 50 eV
 Analyzer Resolution: 0.5 eV
 Emission Angle: 55°
 Total Signal Accumulation Time: 613 s
 Total Elapsed Time: 782 s
 Number of Scans: 10
 Source Beam Size at Specimen Surface: 0.3 mm \times 0.523 mm
 Effective Detector Width: 6.6 eV
 Analyzer Width: 750 μ m \times 6000 μ m

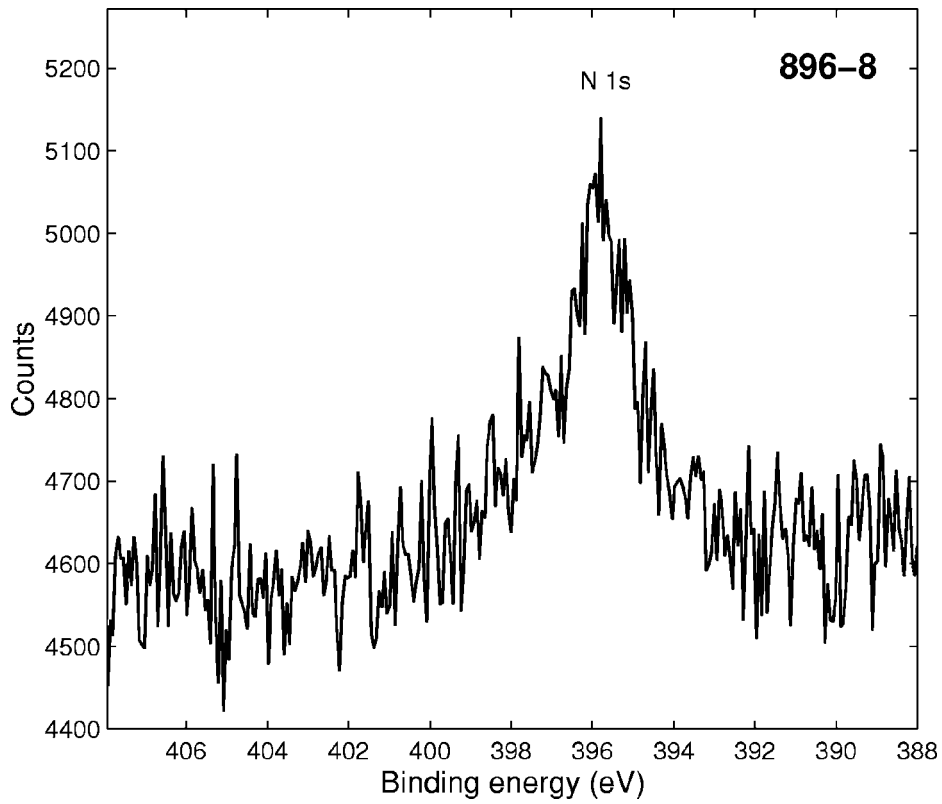

- **Accession #:** 00896-08
- **Host Material:** grain screenings
- **Technique:** XPS
- **Spectral Region:** N 1s

Instrument: Surface Science
Instruments SSX-100

Excitation Source: Al K_{α}
monochromatic

Source Energy: 1486.6 eV

Source Strength: 200 W

Source Size: 0.3 mm \times 0.3 mm

Incident Angle: 55°

Analyzer Type: spherical sector

Analyzer Pass Energy: 50 eV

Analyzer Resolution: 0.5 eV

Emission Angle: 55°

Total Signal Accumulation Time:
22068 s

Total Elapsed Time: 22237 s

Number of Scans: 360

Source Beam Size at Specimen
Surface: 0.3 mm \times 0.523 mm

Effective Detector Width: 6.6 eV

Analyzer Width: 750 μ m \times
6000 μ m